Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Liberty Alpacas/Lorrie Williamson
20014 SE 240th
Maple Valley WA 98038

06/30/16


Test No: 925596

Animal and Sample Description

Animal Name:	Patagonia's Feliciana (2016)	**Animal ID:**	32496871
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	XXXXX	**Sample Date:**	XX/XX/XX
Color:	XXXXX	**Age:**	06/10/12

Laboratory Data

Mean Fiber Diameter:	16.5	microns
Standard Deviation:	3.6	microns
Coefficient of Variation:	21.5	%
Fibers Greater Than 30 microns:	0.5	%

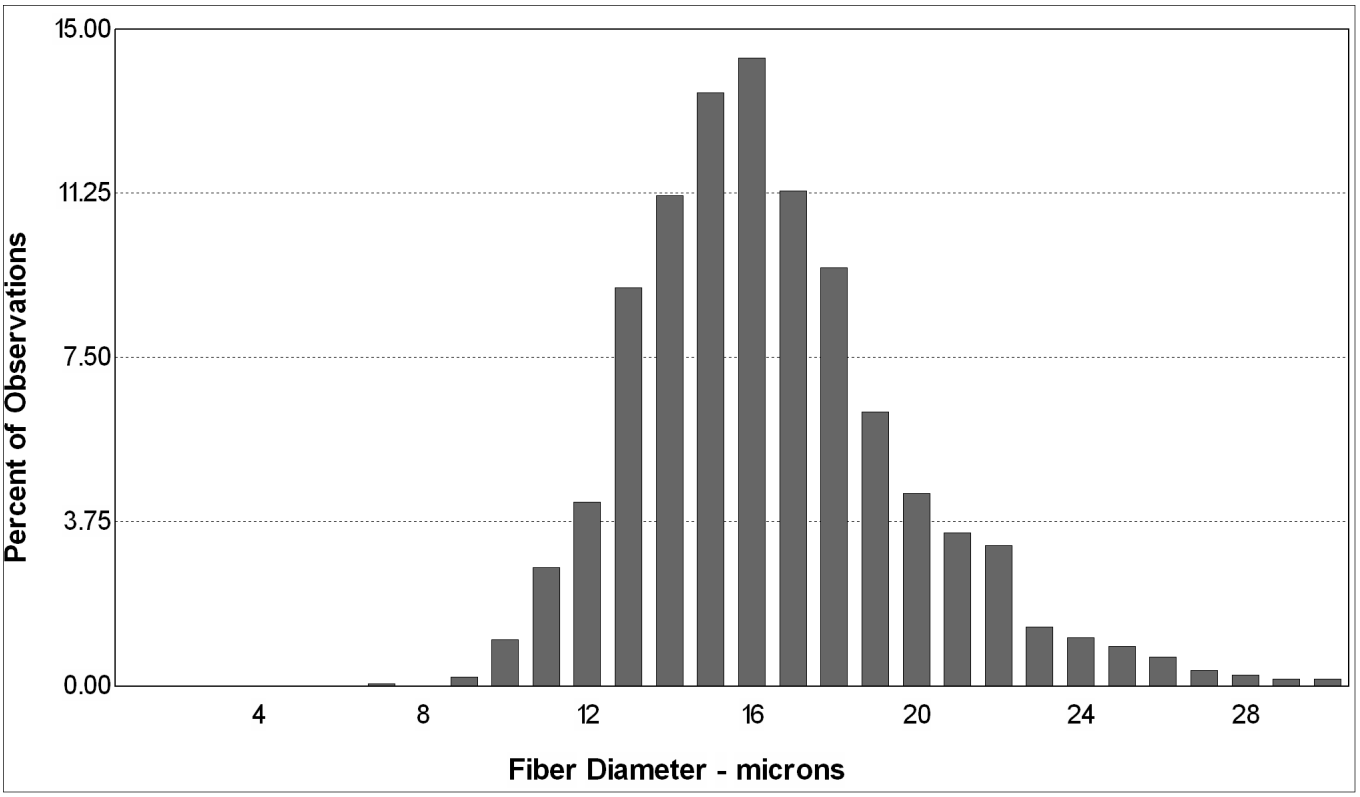

This Test Performed According to I.W.T.O Method 12