Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Skyline Alpacas/Mary Jaffe
11100 NW Saltzman Rd
Portland OR 97229 USA

09/28/11


Test No: 419491

Animal and Sample Description

Animal Name:	Danny Boy	**Animal ID:**	31973281
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Male	**Sample Date:**	04/26/11
Color:	XXXXX	**Age:**	05/29/10

Laboratory Data

Mean Fiber Diameter:	16.5 microns
Standard Deviation:	3.2 microns
Coefficient of Variation:	19.3 %
Fibers Greater Than 30 microns:	0.6 %

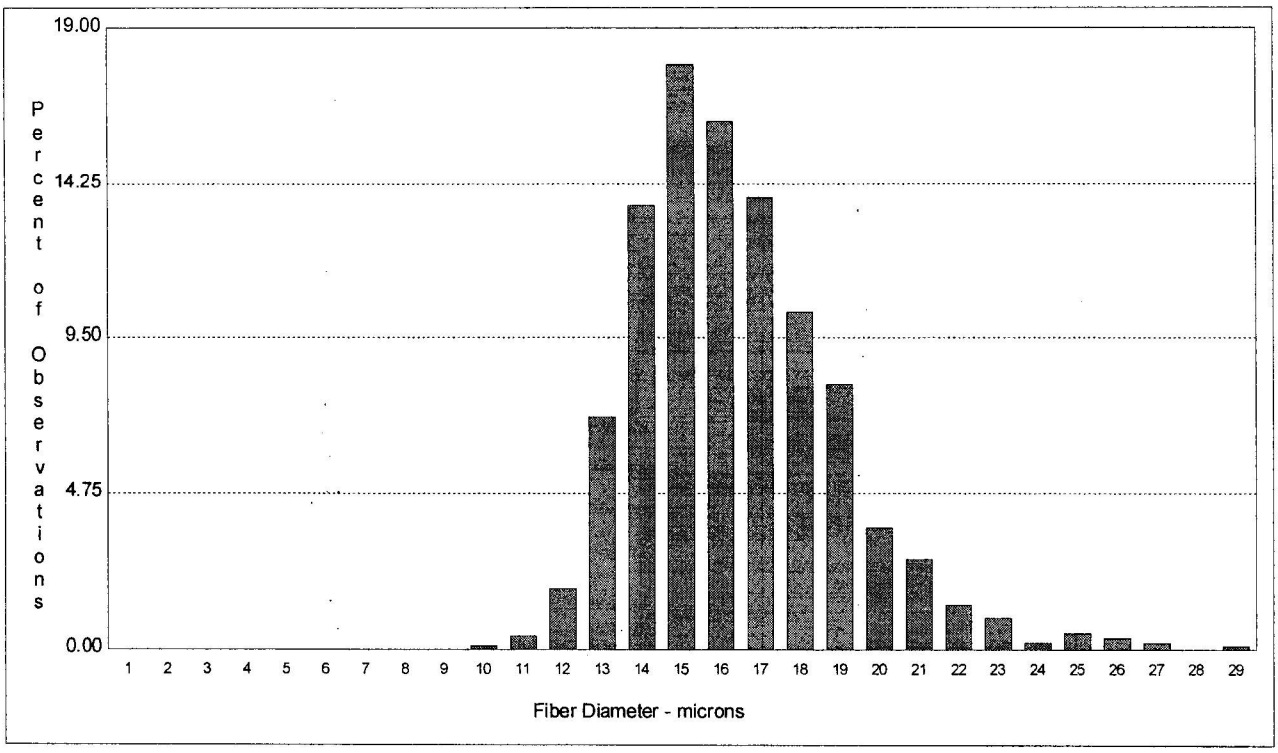

This Test Performed According to I.W.T.O Method 12