Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Skyline Alpacas/Mary Jaffe
11100 NW Saltzman Rd
Portland OR 97229 USA

07/08/16


Test No: 926388

Animal and Sample Description

Animal Name:	Intrigue	**Animal ID:**	32821949
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Female	**Sample Date:**	05/11/16
Color:	Med Silver Grey	**Age:**	08/06/15

Laboratory Data

Mean Fiber Diameter:	16.1	microns
Standard Deviation:	3.6	microns
Coefficient of Variation:	22.4	%
Fibers Greater Than 30 microns:	0.6	%

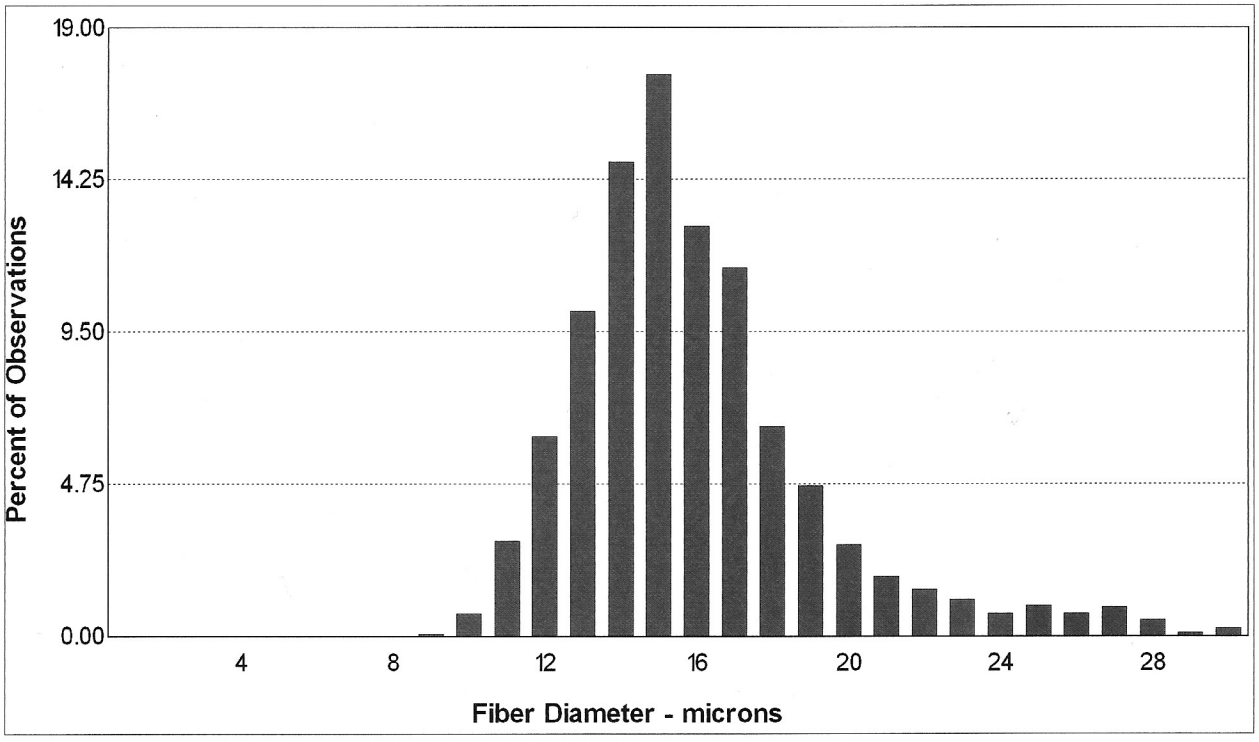

This Test Performed According to I.W.T.O Method 12