



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault
411 Brill Road
West Bolton QC J0E 2T0 Canada

Date: 06/10/14

Test No: 478844


Animal and Sample Description

Animal Name: Ariya Shanghigh's Halle
Breed: Alpaca(Huacaya)
Sex: Female
Color: XXXXX

Animal ID: 32552188
Sample Location: Side
Sample Date: 05/01/14
Age: 07/14/12

Laboratory Data

Mean Fiber Diameter:	20.5 microns	Fibers Greater Than 30 microns:	1.5 %
Standard Deviation:	3.5 microns	Comfort Factor:	98.5 %
Coefficient of Variation:	17.1 %	Mean Curvature:	41.7 deg/mm
Spin Fineness:	19.3 microns	SD Curvature:	22.7 deg/mm

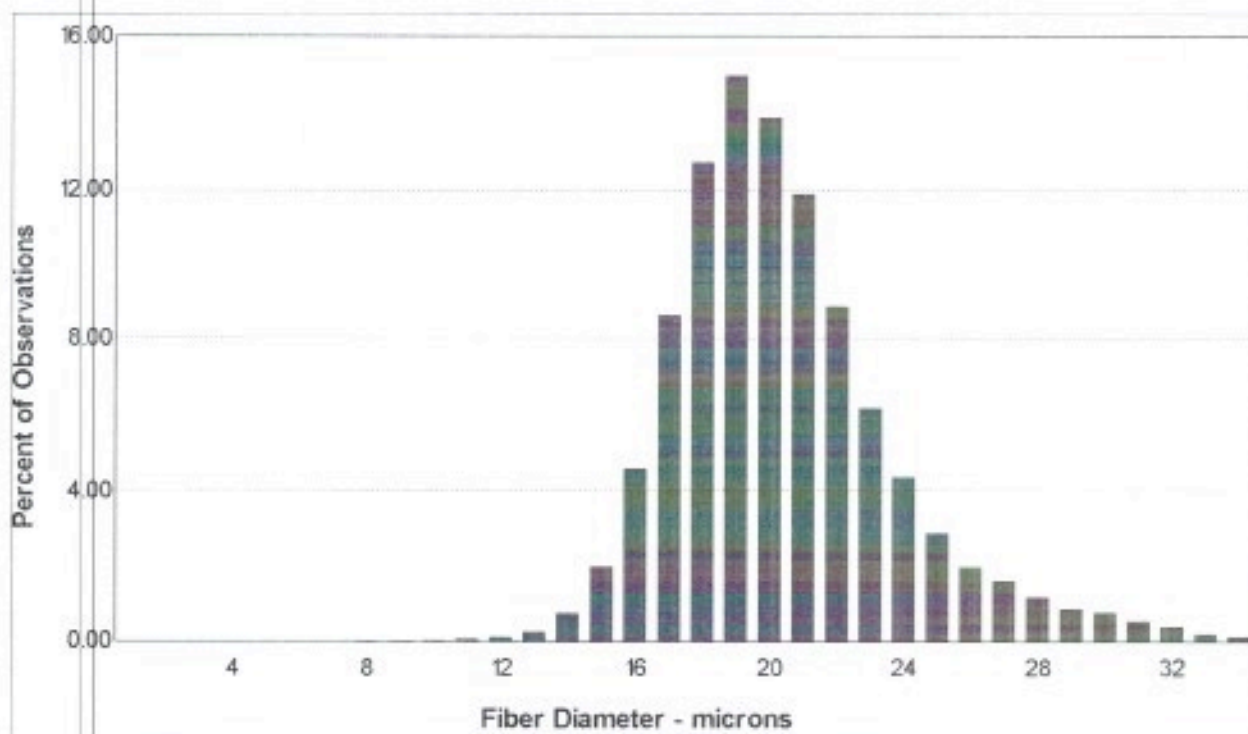

This Test Performed According to I.W.T.O Method 47