Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100)
Micron Test Report

Hy-Haven Farm/Debby Filer
516 Johnson Hollow Rd
Cuba NY 14727-9610


Date: 07/26/16
Test No: 926043

Animal and Sample Description

Animal Name:	STF Sequoia by XXXtreme	**Animal ID:**	35266875
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Male	**Sample Date:**	05/19/16
Color:	Bay Black	**Age:**	09/11/15

Laboratory Data

Mean Fiber Diameter:	20.1 microns	**Fibers Greater Than 30 microns:**	1.5 %
Standard Deviation:	3.8 microns	**Comfort Factor:**	98.5 %
Coefficient of Variation:	19.0 %	**Mean Curvature:**	34.9 deg/mm
Spin Fineness:	19.3 microns	**SD Curvature:**	21.4 deg/mm

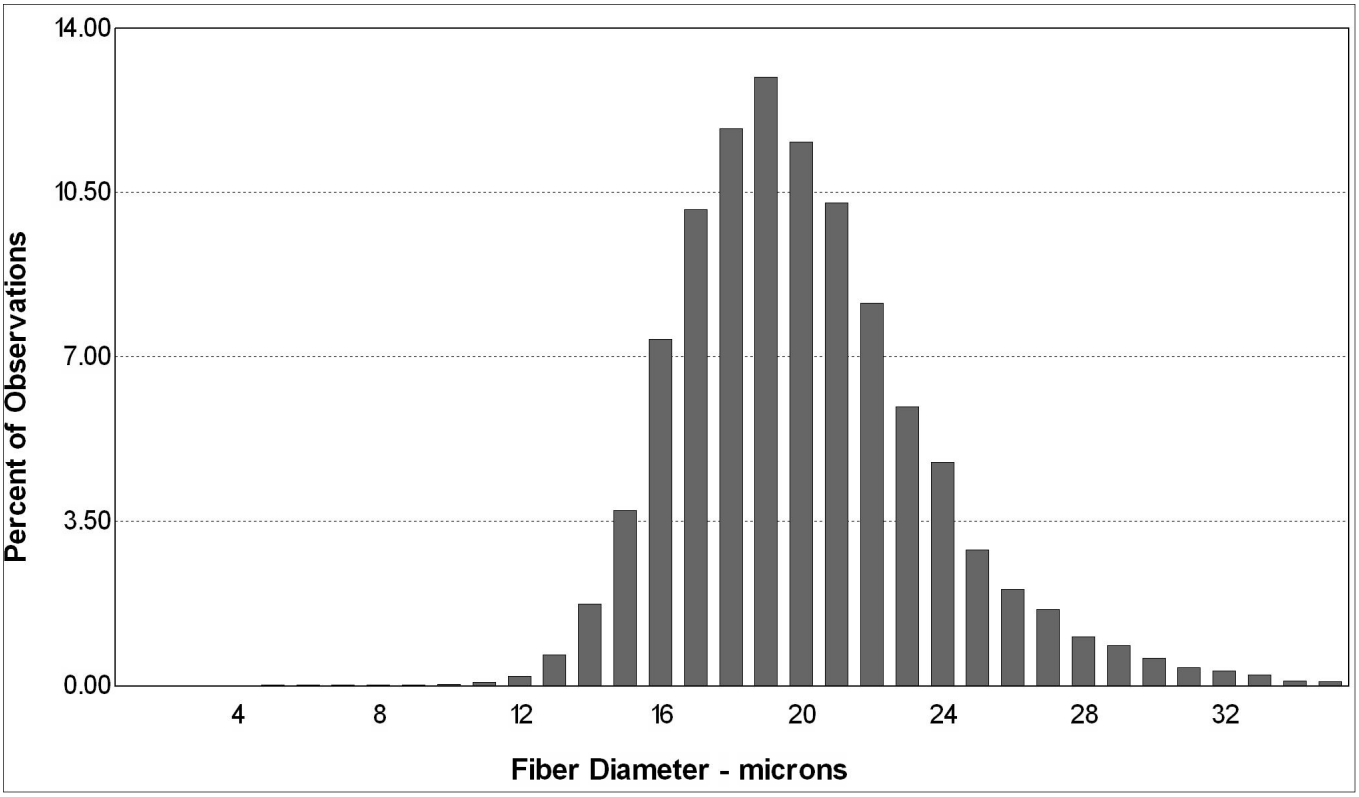

This Test Performed According to I.W.T.O Method 47