Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

B I Bar Ranch/Julie M Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

06/16/18


Test No: 961865

Animal and Sample Description

Animal Name:	BIR's Dotsero	**Animal ID:**	32766684
Breed:	Alpaca(Suri)	**Sample Location:**	Side (R)
Sex:	Female	**Sample Date:**	06/01/18
Color:	White	**Age:**	05/18/14

Laboratory Data

Mean Fiber Diameter:	26.1	microns
Standard Deviation:	4.3	microns
Coefficient of Variation:	16.6	%
Fibers Greater Than 30 microns:	13.6	%

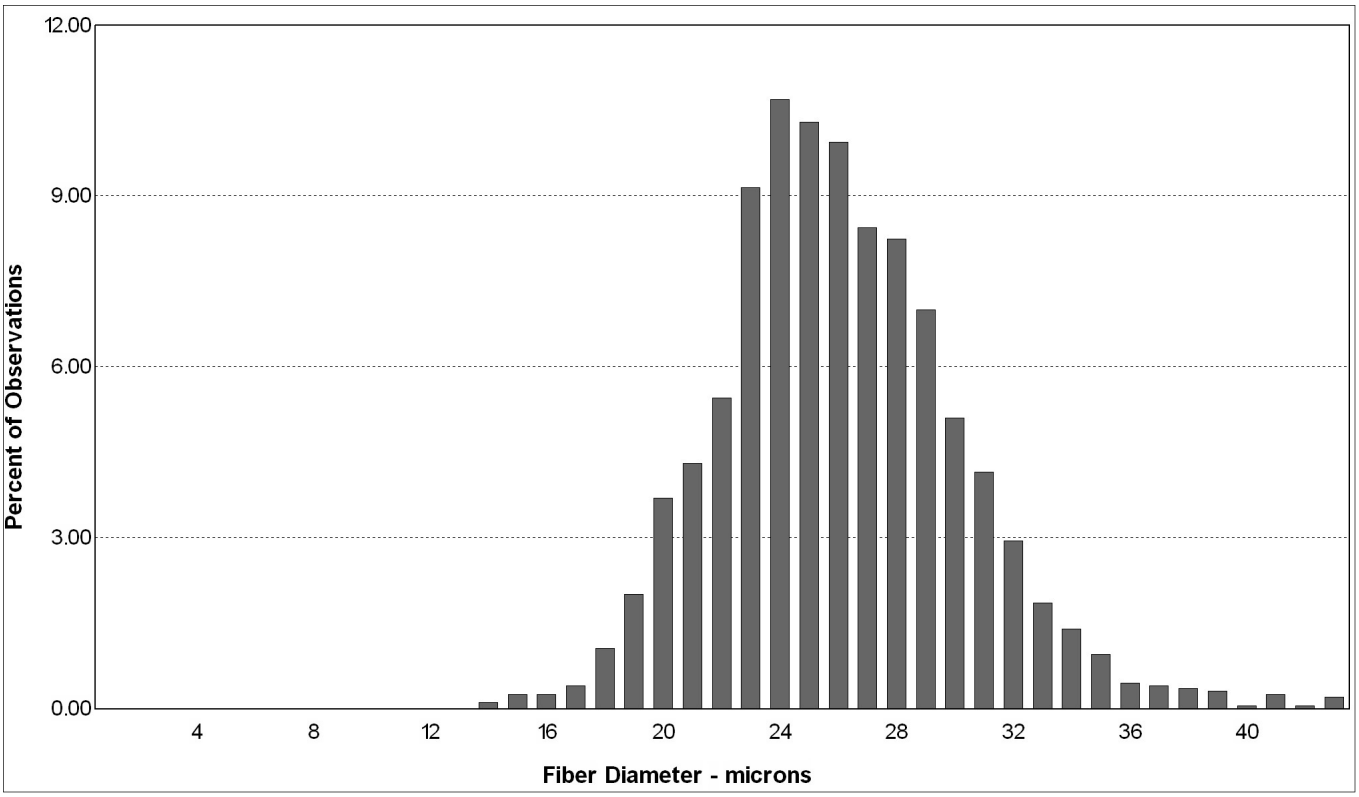

This Test Performed According to I.W.T.O Method 12