Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

B I Bar Ranch/Julie Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

07/19/17


Test No: 945761

Animal and Sample Description

Animal Name:	Lightening	**Animal ID:**	XXXXX
Breed:	Alpaca(Suri)	**Sample Location:**	Side (R)
Sex:	Male	**Sample Date:**	06/01/17
Color:	White	**Age:**	09/05/16

Laboratory Data

Mean Fiber Diameter:	21.0	microns
Standard Deviation:	4.5	microns
Coefficient of Variation:	21.5	%
Fibers Greater Than 30 microns:	3.8	%

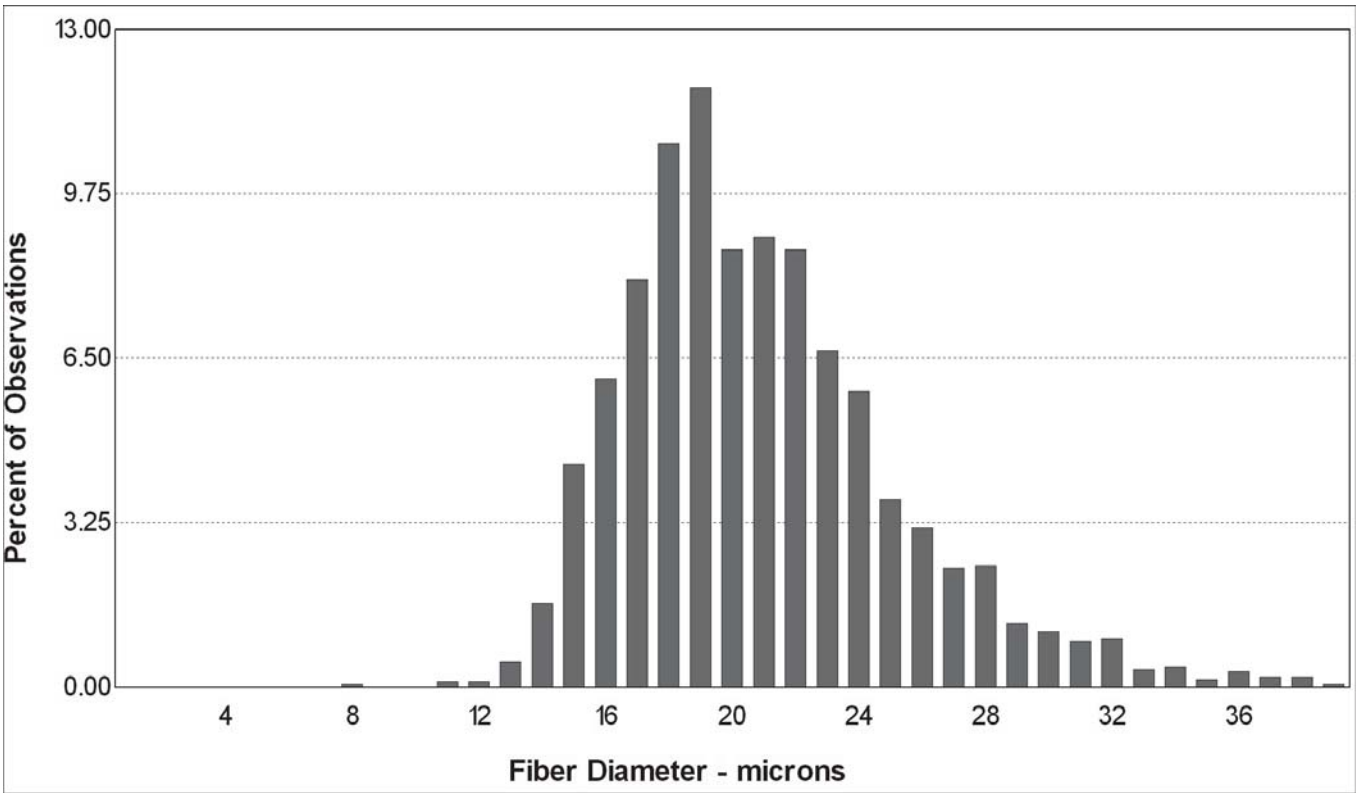

This Test Performed According to I.W.T.O Method 12