Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

B I Bar Ranch/Julie Ritschard
8720 Moss Rock Rd
Colorado Springs CO 80908 USA

06/24/13


Test No: 458377

Animal and Sample Description

Animal Name:	Zebulon	**Animal ID:**	32213027
Breed:	Alpaca(Suri)	**Sample Location:**	Side (R)
Sex:	Male	**Sample Date:**	05/30/13
Color:	Fawn	**Age:**	07/27/12

Laboratory Data

Mean Fiber Diameter:	20.0	microns
Standard Deviation:	4.0	microns
Coefficient of Variation:	20.1	%
Fibers Greater Than 30 microns:	2.6	%

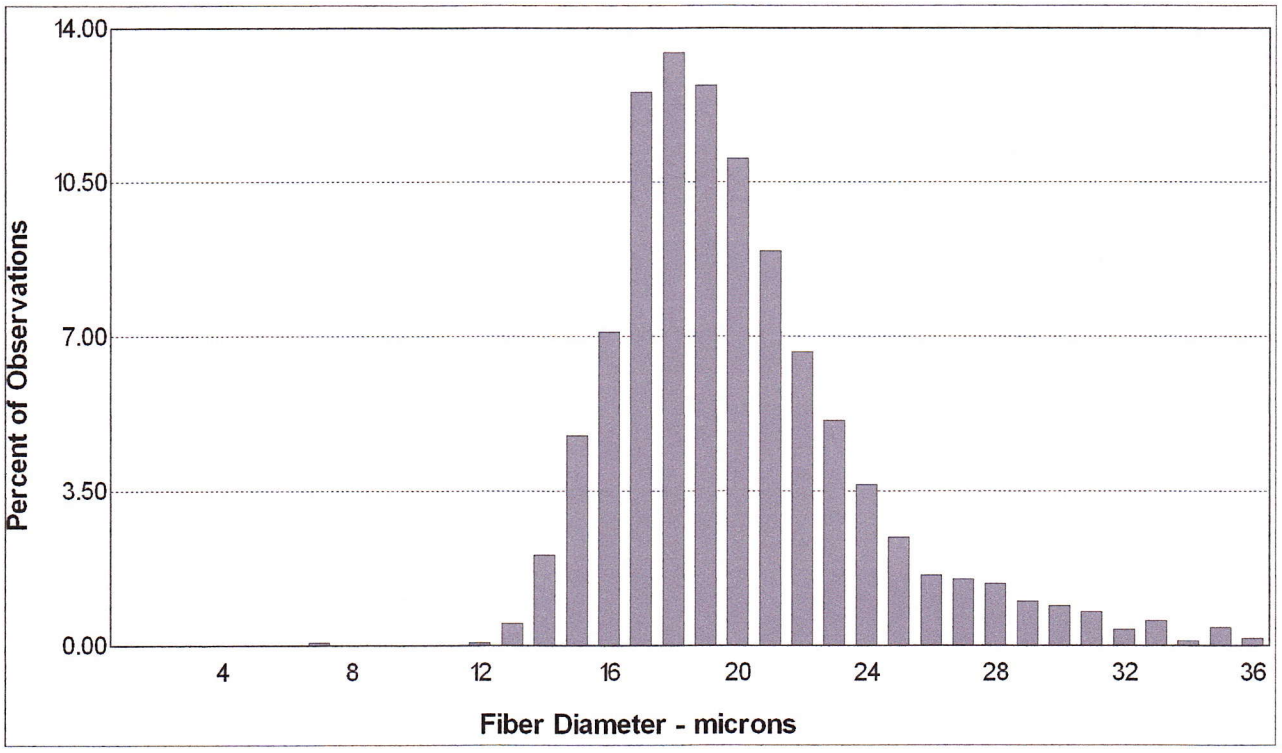

This Test Performed According to I.W.T.O Method 12