Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

K-Ran Alpacas/Randy Strong
11579 Wessie Rd
Prattsburgh NY 14873 USA

06/14/12


Test No: 431568

Animal and Sample Description

Animal Name:	Jack	**Animal ID:**	XXXXX
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side (R)
Sex:	Male	**Sample Date:**	05/03/12
Color:	Fawn	**Age:**	XXXXX

Laboratory Data

Mean Fiber Diameter:	17.4 microns
Standard Deviation:	3.5 microns
Coefficient of Variation:	20.2 %
Fibers Greater Than 30 microns:	0.6 %

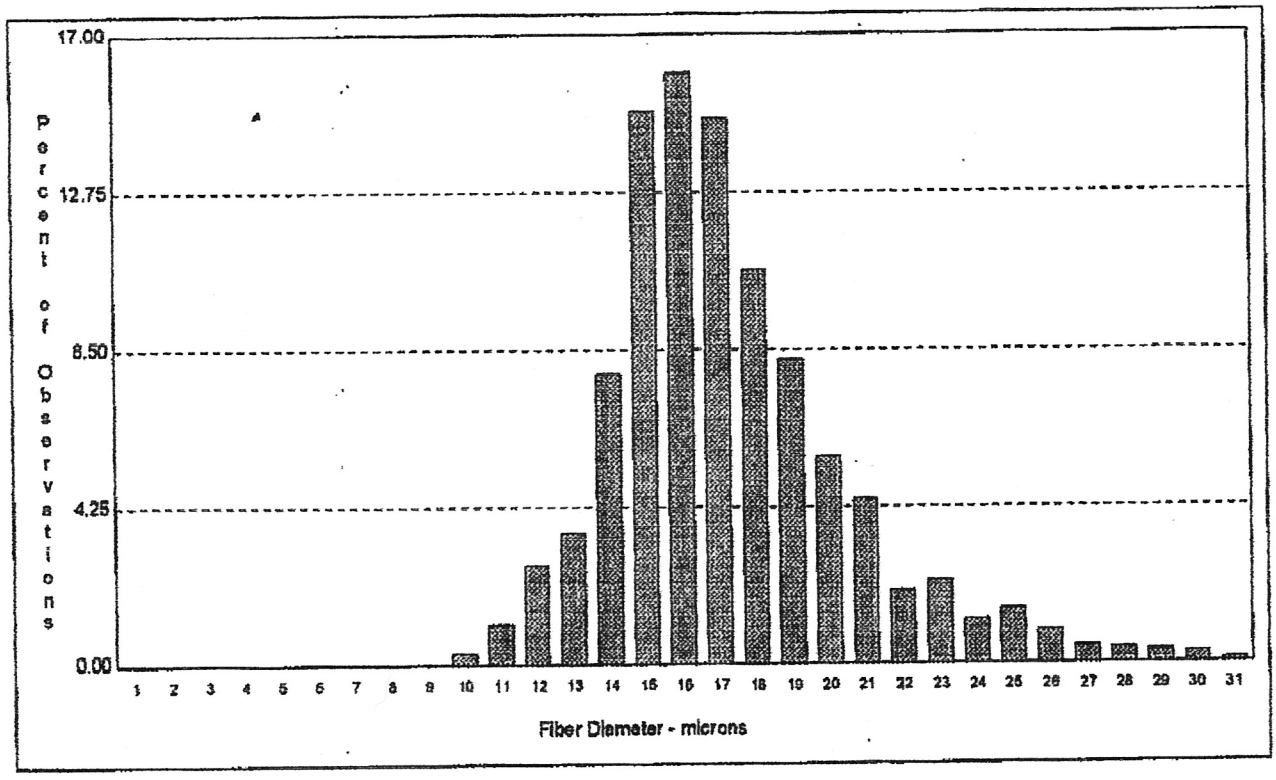

This Test Performed According to I.W.T.O Method 12