



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Seldom Scene Farm/Paul & Lindy Huber
1710 Watts Ferry Rd
Frankfort KY 40601 U.S.A.

02/11/08

Test No: 316847


Animal and Sample Description

Animal Name: SSF Accoyo Optimist
Breed: Alpaca(Huacaya)
Sex: XXXXX
Color: XXXXX

Animal ID: XXXXX
Sample Location: Side
Sample Date: XX/XX/XX
Age: 10 Mos

Laboratory Data

Mean Fiber Diameter: 19.2 microns
Standard Deviation: 3.5 microns
Coefficient of Variation: 18.2 %
Fibers Greater Than 30 microns: 0.7 %

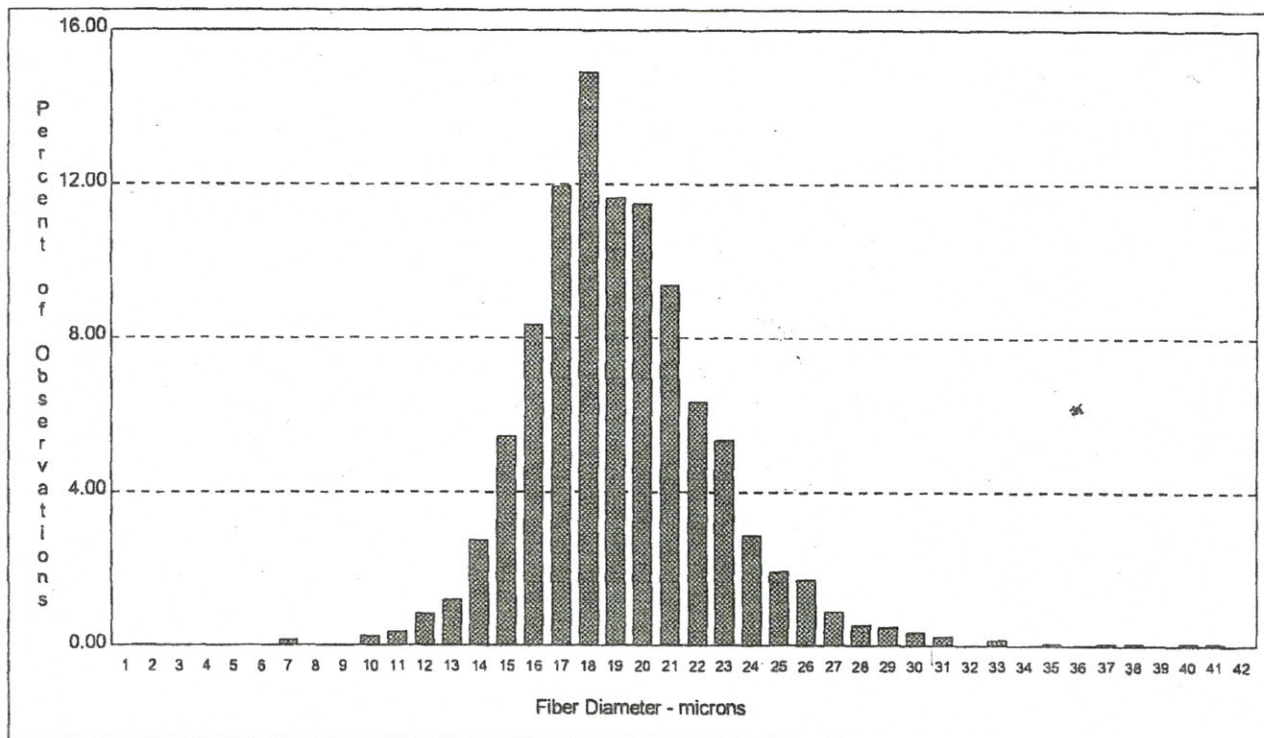

This Test Performed According to I.W.T.O Method 12