Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Stachowski Alpacas, LLC/Anthony Stachowski DVM
P.O. Box 828
Mantua OH 44255

12/16/19


Test No: 986631

Animal and Sample Description

Animal Name:	862 MATARO	**Animal ID:**	862
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Male	**Sample Date:**	12/07/19
Color:	True Black	**Age:**	10/14/18

Laboratory Data

Mean Fiber Diameter:	19.7	microns
Standard Deviation:	3.9	microns
Coefficient of Variation:	19.7	%
Fibers Greater Than 30 microns:	1.8	%

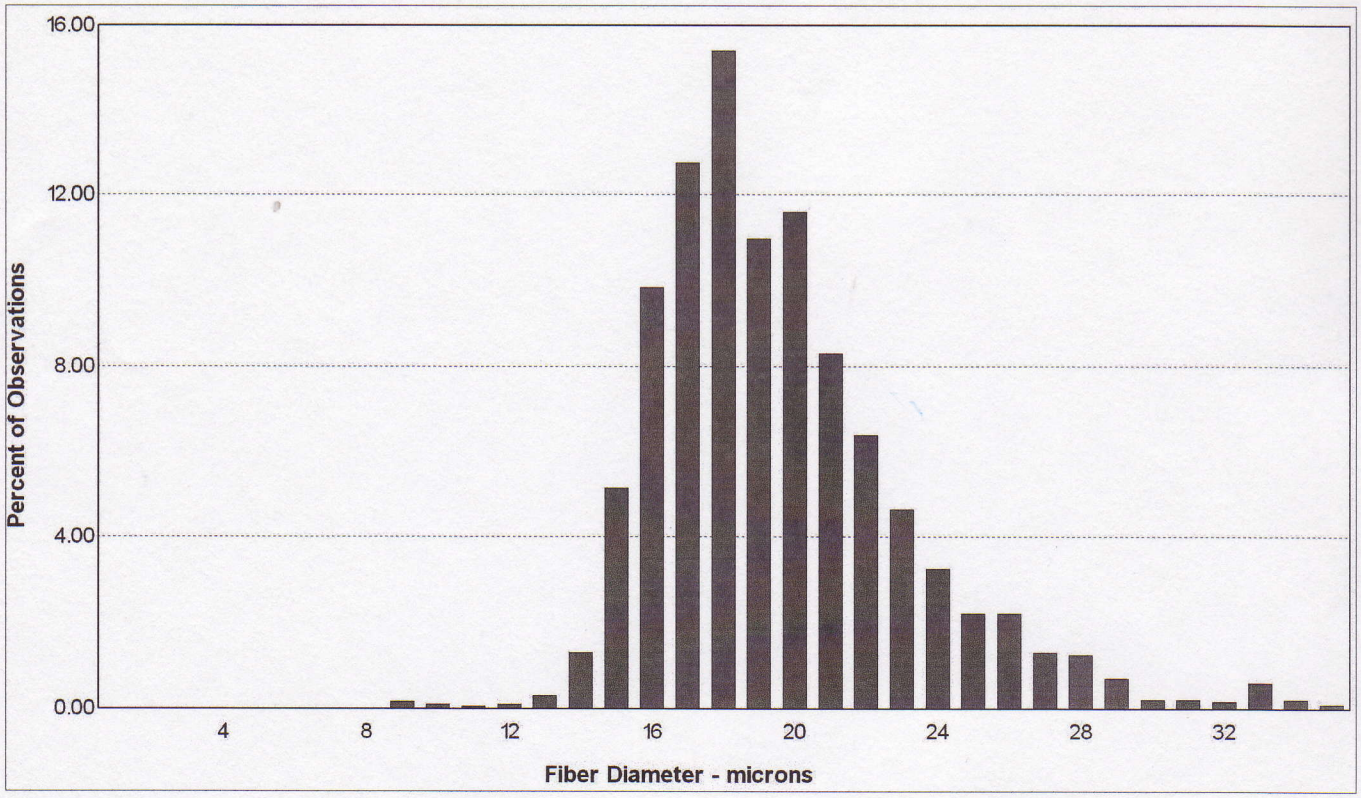

This Test Performed According to I.W.T.O Method 12