Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100)
Micron Test Report

Alpacas of Moose Creek Ranch/Debbie Hoerl
23681 Quivira Road
Bucyrus KS 66013


Date: 06/19/19
Test No: 975936

Animal and Sample Description

Animal Name:	Irish Meadows Aubrey	**Animal ID:**	35258438
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Female	**Sample Date:**	04/23/2019
Color:	Med Fawn	**Age:**	08/30/2015

Laboratory Data

Mean Fiber Diameter:	19.7 microns	**Fibers Greater Than 30 microns:**	2.1 %
Standard Deviation:	4.0 microns	**Comfort Factor:**	97.9 %
Coefficient of Variation:	20.3 %	**Mean Curvature:**	44.1 deg/mm
Spin Fineness:	19.1 microns	**SD Curvature:**	22.1 deg/mm

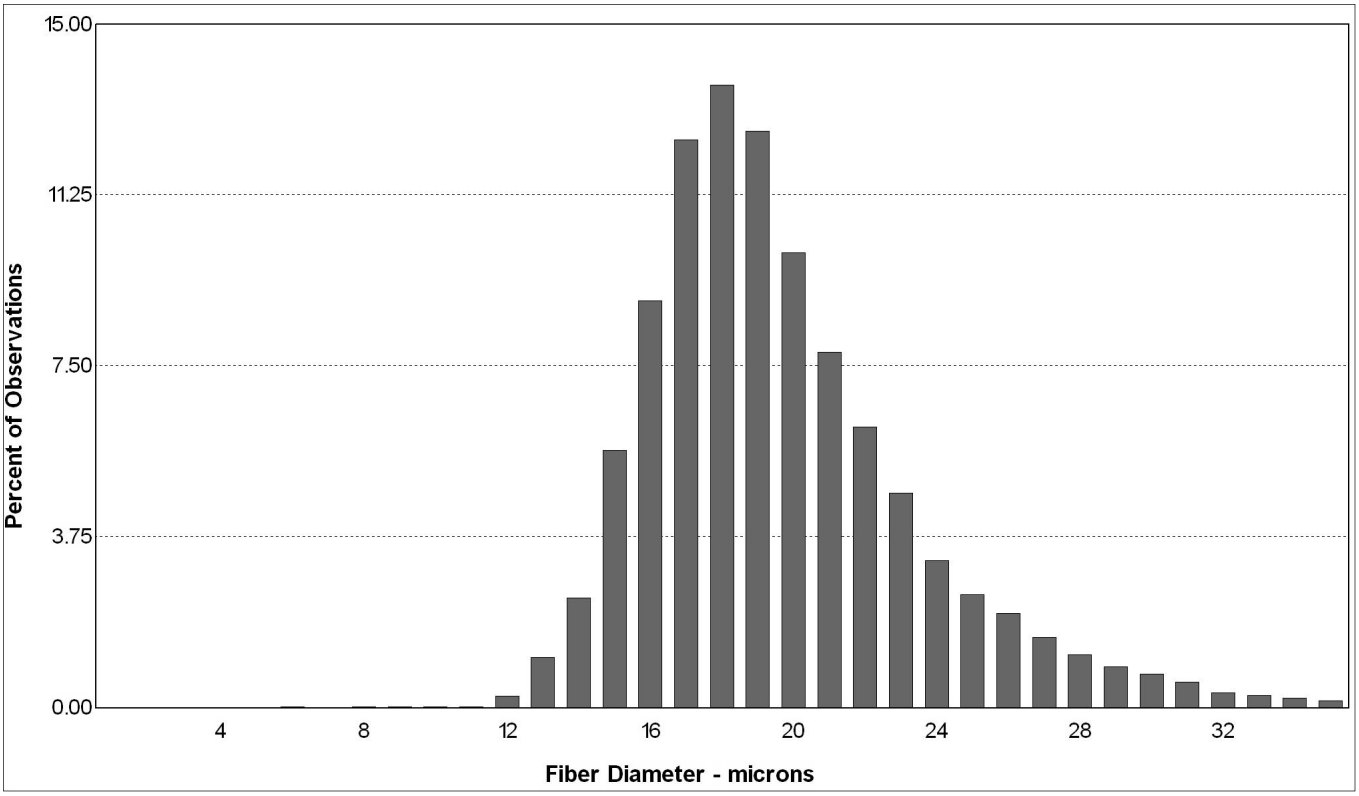

This Test Performed According to I.W.T.O Method 47