Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Starshire Ranch/June Aploks
8300 Robbins Rd
Ellensburg WA 98926 USA

06/30/12


Test No: 432392

Animal and Sample Description

Animal Name:	Love Sonnet	**Animal ID:**	31691666
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Female	**Sample Date:**	05/19/12
Color:	Silver Gray	**Age:**	09/04/09

Laboratory Data

Mean Fiber Diameter:	18.3 microns	**Spin Fineness:**	18.5 microns
Standard Deviation:	4.6 microns	**Mean Curvature (deg/mm):**	49.8
Coefficient of Variation:	24.9 %	**SD Curvature (deg/mm):**	27.2
Fibers Greater Than 30 microns:	2.2 %	**Comfort Factor:**	97.8 %

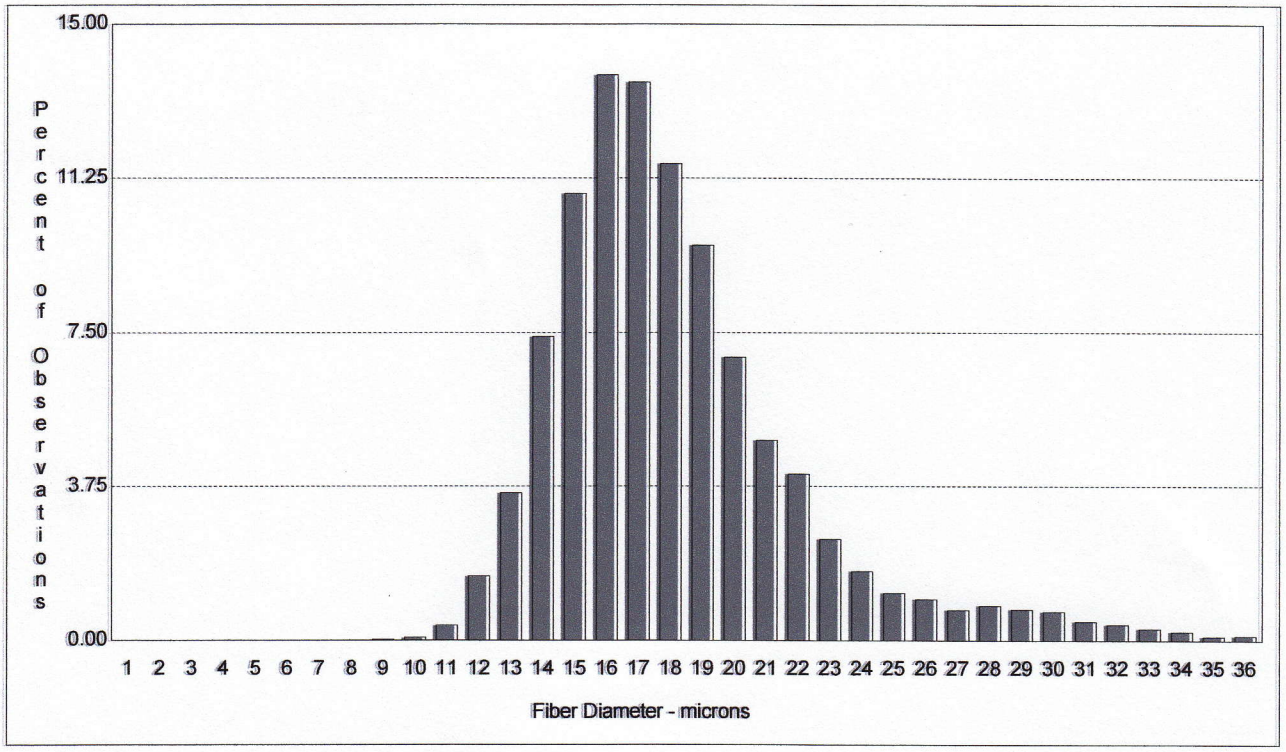

This Test Performed According to I.W.T.O Method 47