Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Hubbert Farms/Kathy McConnell
600 Lily Lake Rd
Peterborough ON K9J 6X3 Canada

09/29/11


Test No: 419553

Animal and Sample Description

Animal Name:	Fantasia of Peterboro	**Animal ID:**	31935395
Breed:	Alpaca(Huacaya)	**Sample Location:**	Blanket
Sex:	Female	**Sample Date:**	05/10/11
Color:	Brown	**Age:**	06/20/10

Laboratory Data

Mean Fiber Diameter:	20.5 microns	**Spin Fineness:**	20.0 microns
Standard Deviation:	4.3 microns	**Mean Curvature (deg/mm):**	32.9
Coefficient of Variation:	21.0 %	**SD Curvature (deg/mm):**	21.5
Fibers Greater Than 30 microns:	3.1 %	**Comfort Factor:**	96.9 %

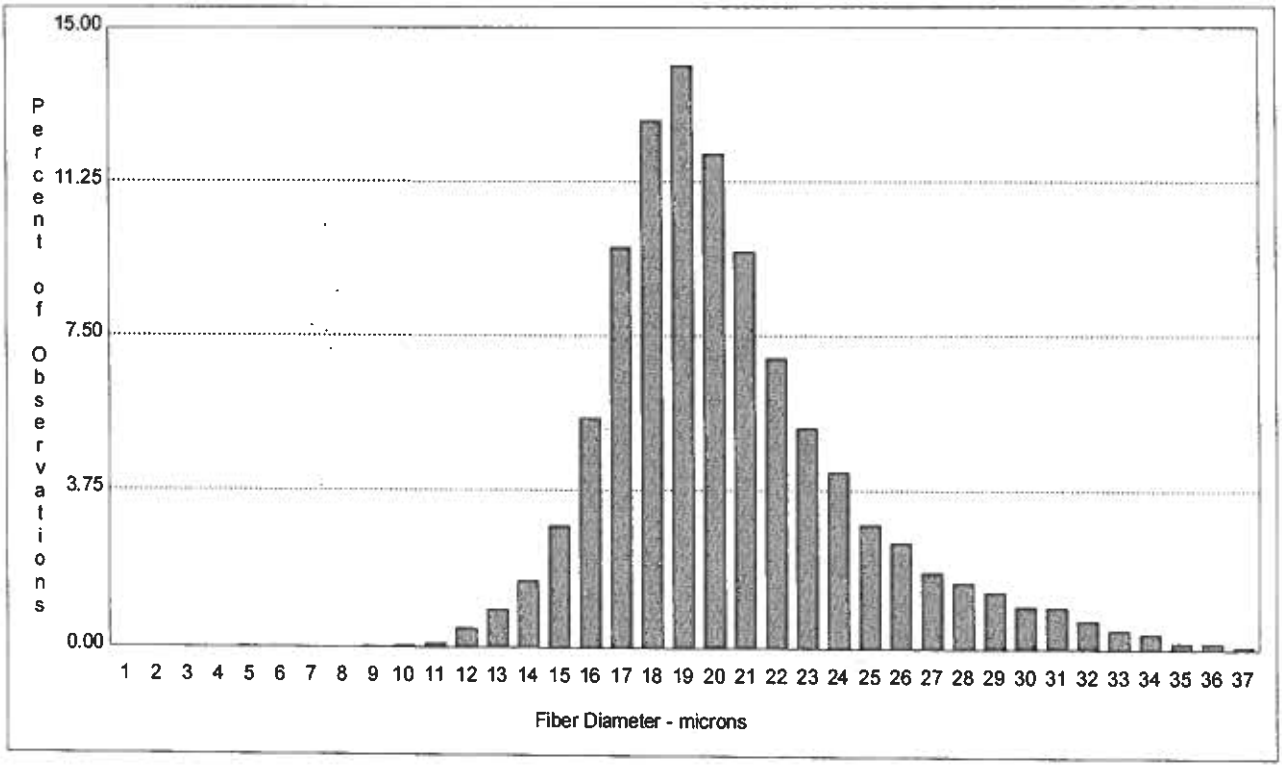

This Test Performed According to I.W.T.O Method 47