Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Miller-McMahan Alpacas/Candace McMahan
1897 Ashland Road
Ruffin NC 27326 USA

05/20/15


Test No: 900857

Animal and Sample Description

Animal Name:	MMALP Beau's Devaro	**Animal ID:**	32546590
Breed:	Alpaca(Suri)	**Sample Location:**	Side
Sex:	Male	**Sample Date:**	05/03/15
Color:	True Black	**Age:**	05/23/13

Laboratory Data

Mean Fiber Diameter:	19.2 microns
Standard Deviation:	4.8 microns
Coefficient of Variation:	24.9 %
Fibers Greater Than 30 microns:	3.2 %

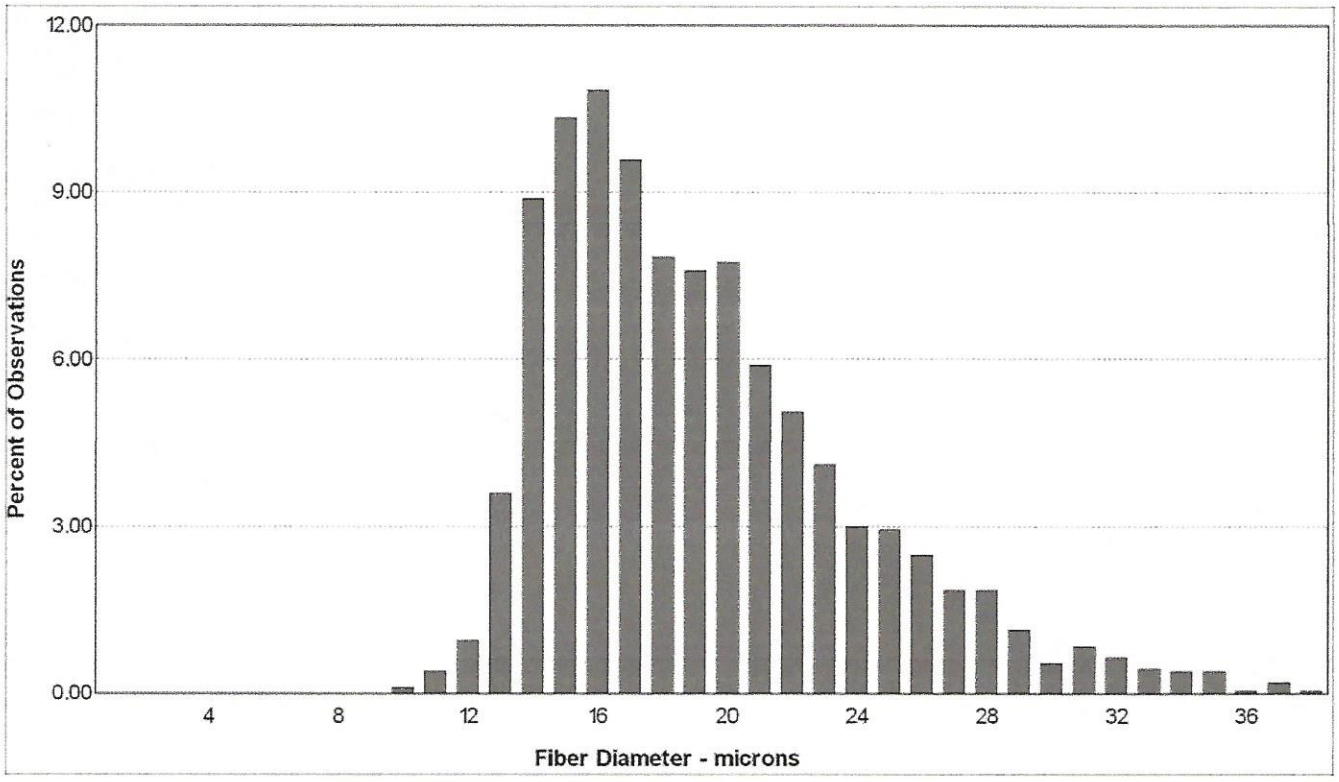

This Test Performed According to I.W.T.O Method 12