

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Bentwood Alpacas/Suzanne & Mark Drumm
P.O. Box 1177
Tully NY 13159 USA

09/08/09

Test No: 363099


Animal and Sample Description

Animal Name: Luna
Breed: Alpaca(Huacaya)
Sex: Female
Color: XXXXX

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/30/09
Age: 06/29/08

Laboratory Data

Mean Fiber Diameter: 17.7 microns
Standard Deviation: 4.0 microns
Coefficient of Variation: 22.6 %
Fibers Greater Than 30 microns: 0.7 %

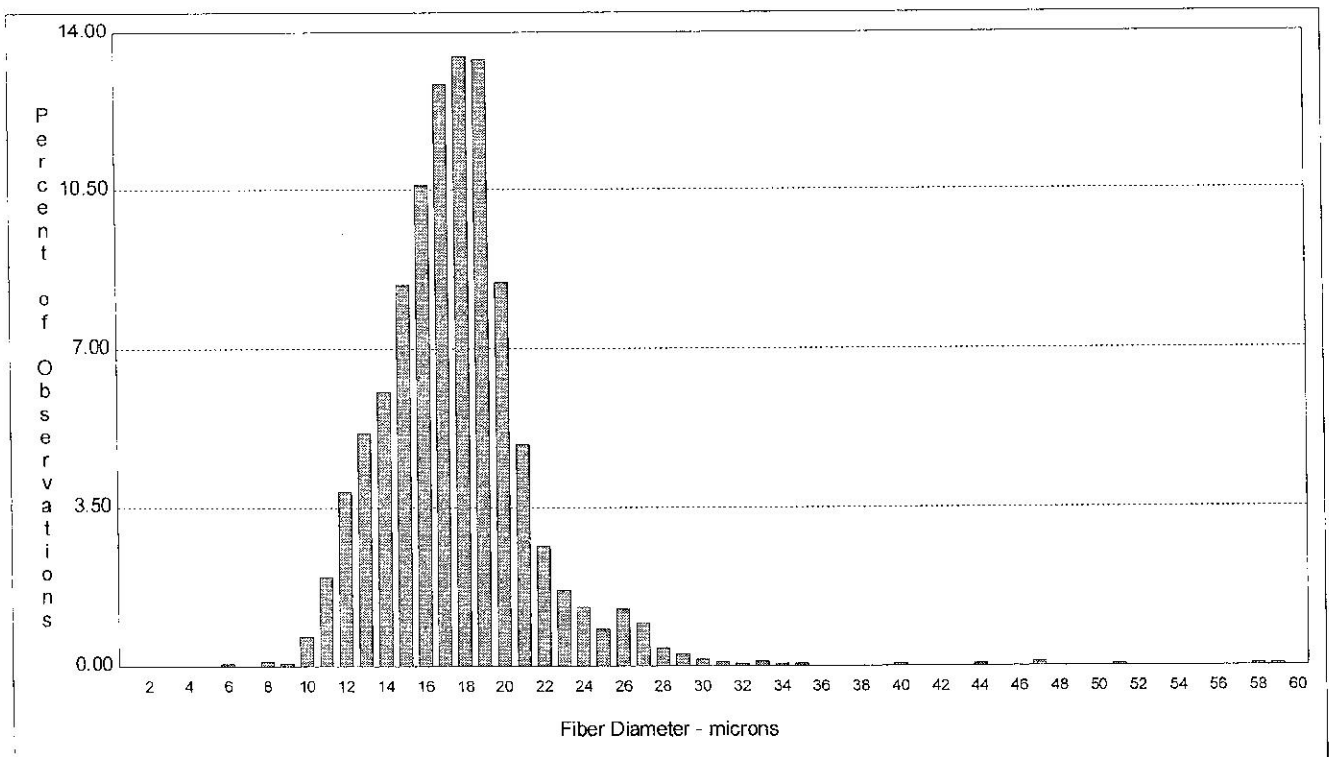

This Test Performed According to I.W.T.O Method 12