Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100)
Micron Test Report

Thordarson Farms/Heather Thordarson
13492 South Warnock Rd
Oregon City OR 97045-9142 USA


Date: 08/16/19
Test No: 981042

Animal and Sample Description

Animal Name:	MJA Crystal Stone	**Animal ID:**	32381979
Breed:	Alpaca(Huacaya)	**Sample Location:**	Mid Side
Sex:	Female	**Sample Date:**	06/09/19
Color:	Med Fawn	**Age:**	09/21/11

Laboratory Data

Mean Fiber Diameter:	23.1 microns	**Fibers Greater Than 30 microns:**	6.4 %
Standard Deviation:	4.7 microns	**Comfort Factor:**	93.6 %
Coefficient of Variation:	20.3 %	**Mean Curvature:**	34.2 deg/mm
Spin Fineness:	22.4 microns	**SD Curvature:**	20.9 deg/mm

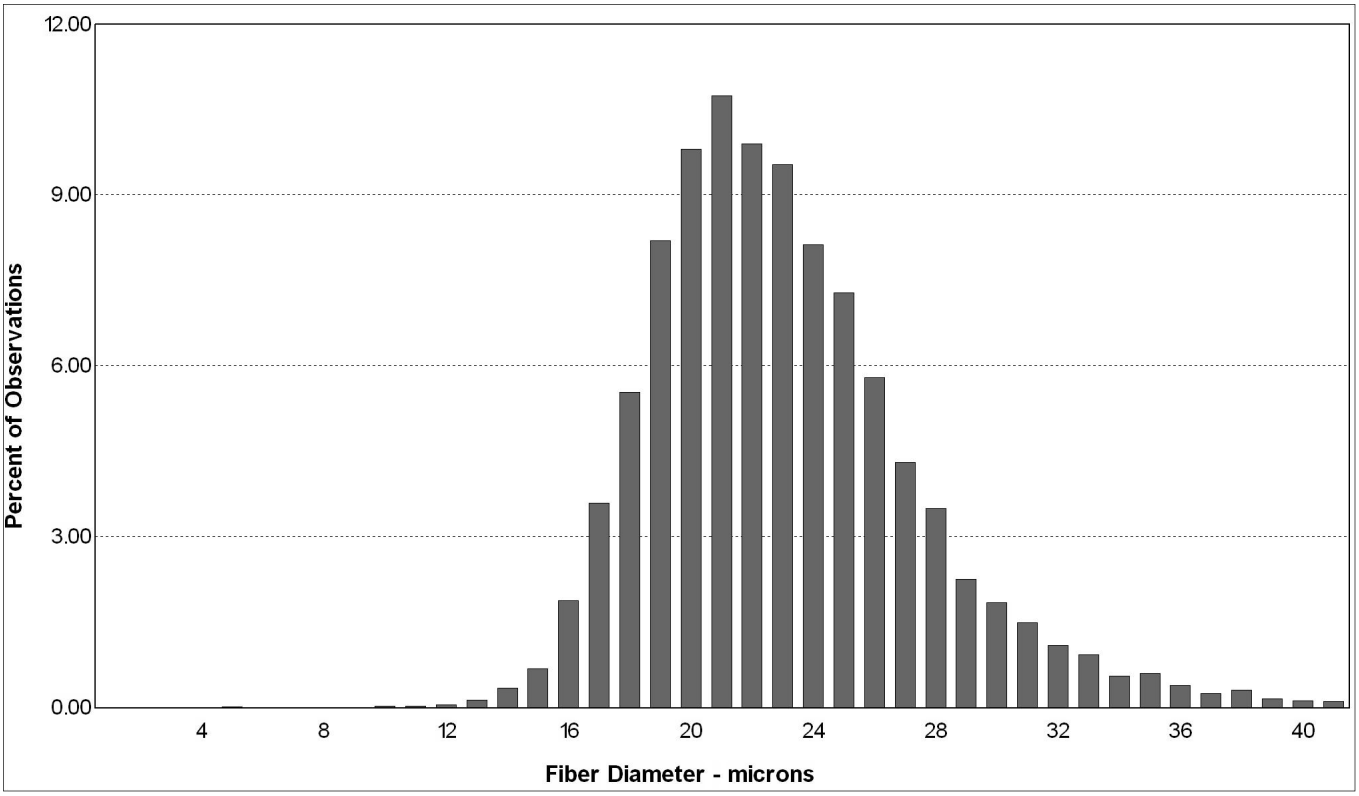

This Test Performed According to I.W.T.O Method 47