Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Cascade Rose Alpacas/Shari Hollinger
1826 324th Avenue NE
Carnation WA 98014 USA

10/11/16


Test No: 936849

Animal and Sample Description

Animal Name:	Cedar Springs Picasso	**Animal ID:**	31376099
Breed:	Alpaca(Huacaya)	**Sample Location:**	Mid Side
Sex:	Male	**Sample Date:**	05/31/16
Color:	Dark Rose Grey	**Age:**	08/21/10

Laboratory Data

Mean Fiber Diameter:	21.9 microns	**Spin Fineness:**	21.9 microns
Standard Deviation:	5.3 microns	**Mean Curvature (deg/mm):**	34.2
Coefficient of Variation:	24.4 %	**SD Curvature (deg/mm):**	23.0
Fibers Greater Than 30 microns:	6.8 %	**Comfort Factor:**	93.2 %

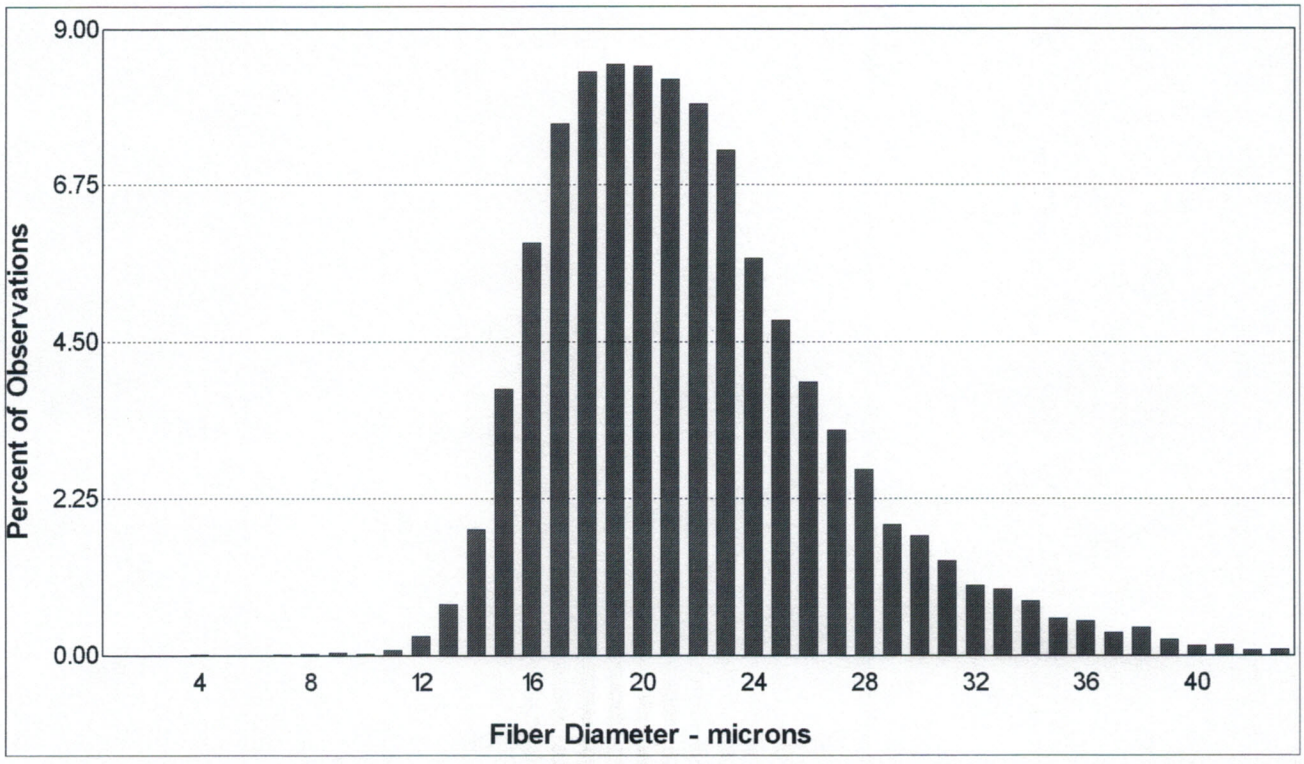

This Test Performed According to I.W.T.O Method 47