Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100)
Micron Test Report

Ten Seven Acres/Jessie Monson
107 Galchutt Ave
Galchutt ND 58075 USA


Date: 08/06/18
Test No: 967019

Animal and Sample Description

Animal Name:	Liam	**Animal ID:**	XXXXX
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Male	**Sample Date:**	05/10/18
Color:	Lt Brown	**Age:**	08/15/17

Laboratory Data

Mean Fiber Diameter:	19.7 microns	**Fibers Greater Than 30 microns:**	3.0 %
Standard Deviation:	4.6 microns	**Comfort Factor:**	97.0 %
Coefficient of Variation:	23.3 %	**Mean Curvature:**	37.2 deg/mm
Spin Fineness:	19.6 microns	**SD Curvature:**	22.5 deg/mm

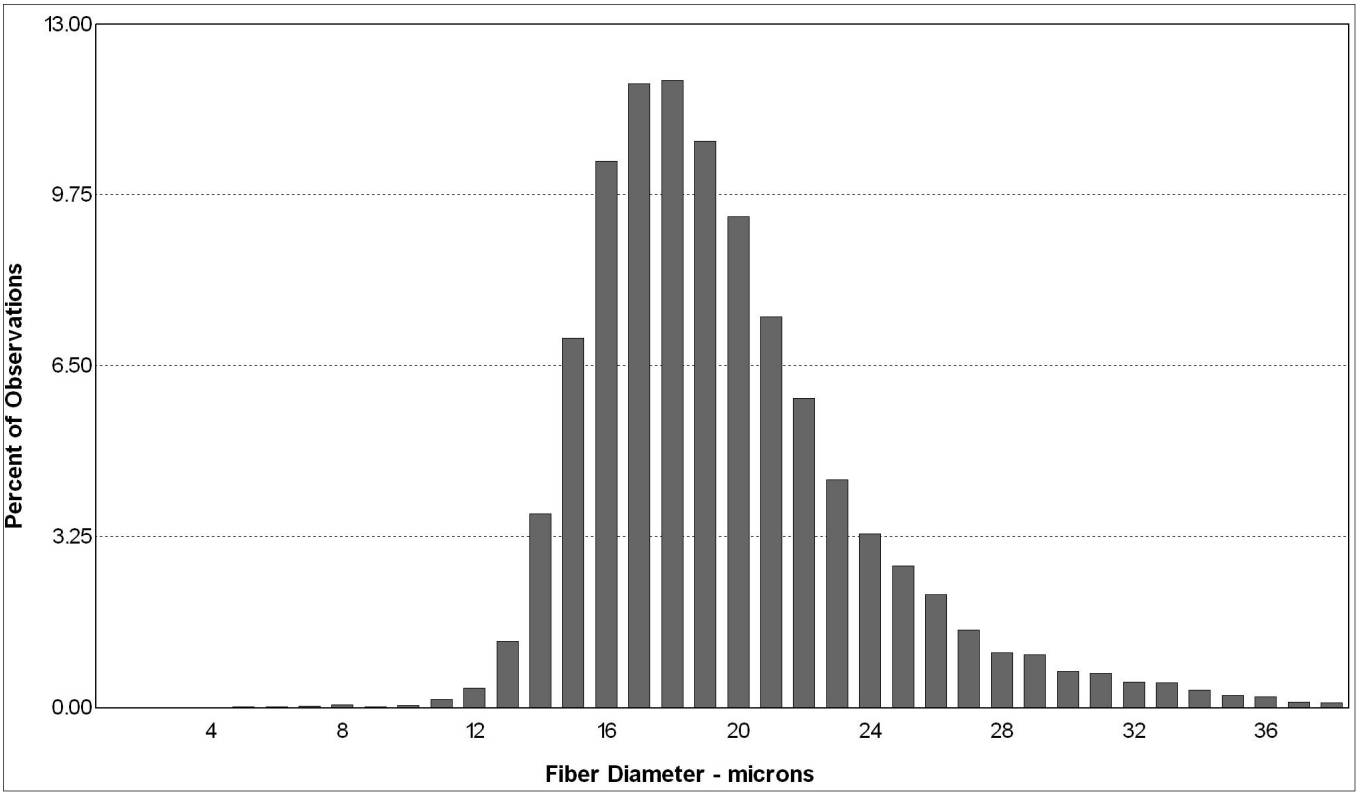

This Test Performed According to I.W.T.O Method 47