Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Man in the Moon Farm, LLC/Brenda Landes & Mark Edmonds
16108 Johns Creek Rd
New Castle VA 24127 USA

09/18/17


Test No: 952451

Animal and Sample Description

Animal Name:	SA Peruvian Alivia	**Animal ID:**	32065121
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Female	**Sample Date:**	05/25/17
Color:	MF	**Age:**	04/05/10

Laboratory Data

Mean Fiber Diameter:	21.0 microns	**Spin Fineness:**	20.1 microns
Standard Deviation:	4.0 microns	**Mean Curvature (deg/mm):**	38.7
Coefficient of Variation:	18.9 %	**SD Curvature (deg/mm):**	23.4
Fibers Greater Than 30 microns:	1.9 %	**Comfort Factor:**	98.1 %

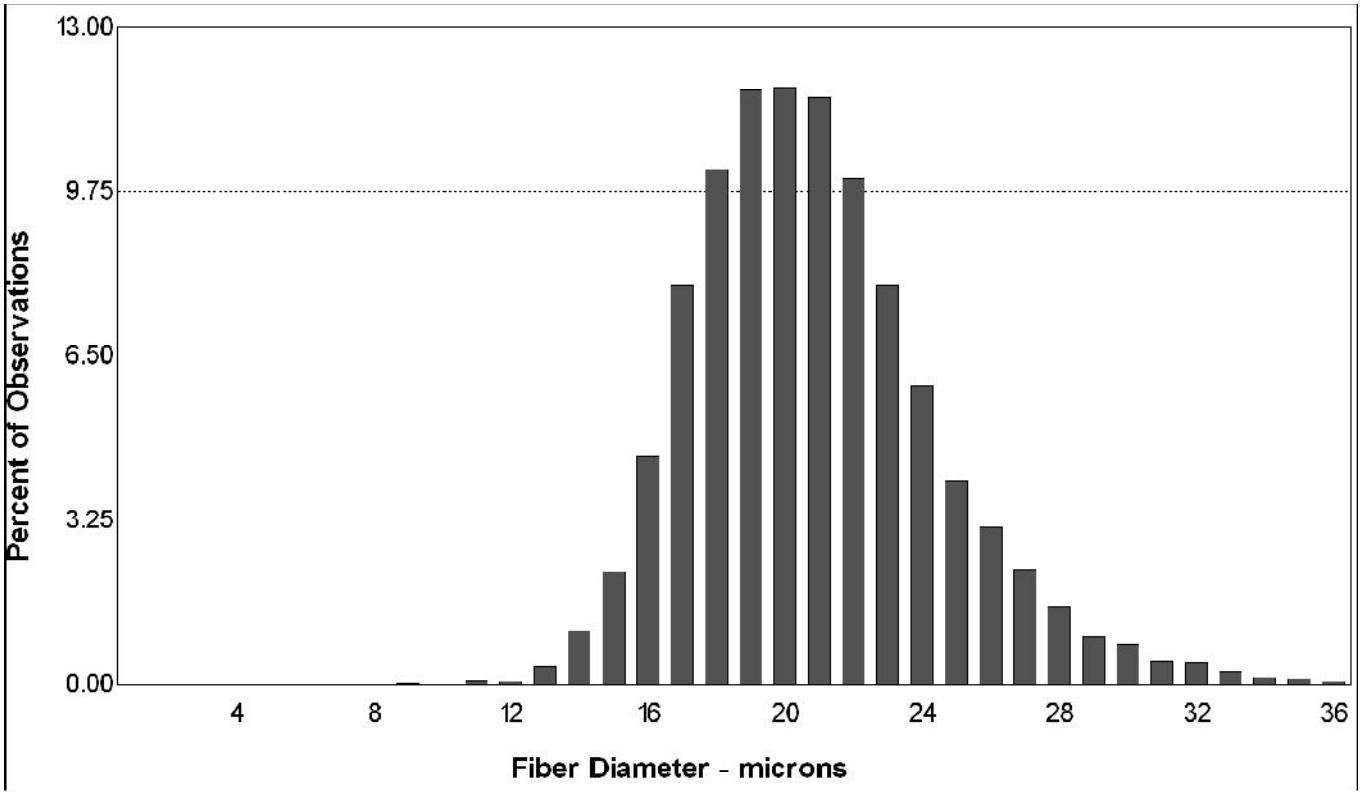

This Test Performed According to I.W.T.O Method 47