Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

MapleView Alpacas/Edwin G Pierrot
8462 Christmiller Rd
Cattaraugus NY 14719 USA

10/02/18

Test No: 970197

Animal and Sample Description

Animal Name:	Maple View's Eclipse	**Animal ID:**	35179733
Breed:	Alpaca(Huacaya)	**Sample Location:**	Blanket
Sex:	Male	**Sample Date:**	05/15/18
Color:	True Black	**Age:**	08/22/17

Laboratory Data

Mean Fiber Diameter:	24.8 microns	**Spin Fineness:**	25.5 microns
Standard Deviation:	6.7 microns	**Mean Curvature (deg/mm):**	24.1
Coefficient of Variation:	26.9 %	**SD Curvature (deg/mm):**	16.3
Fibers Greater Than 30 microns:	15.7 %	**Comfort Factor:**	84.3 %

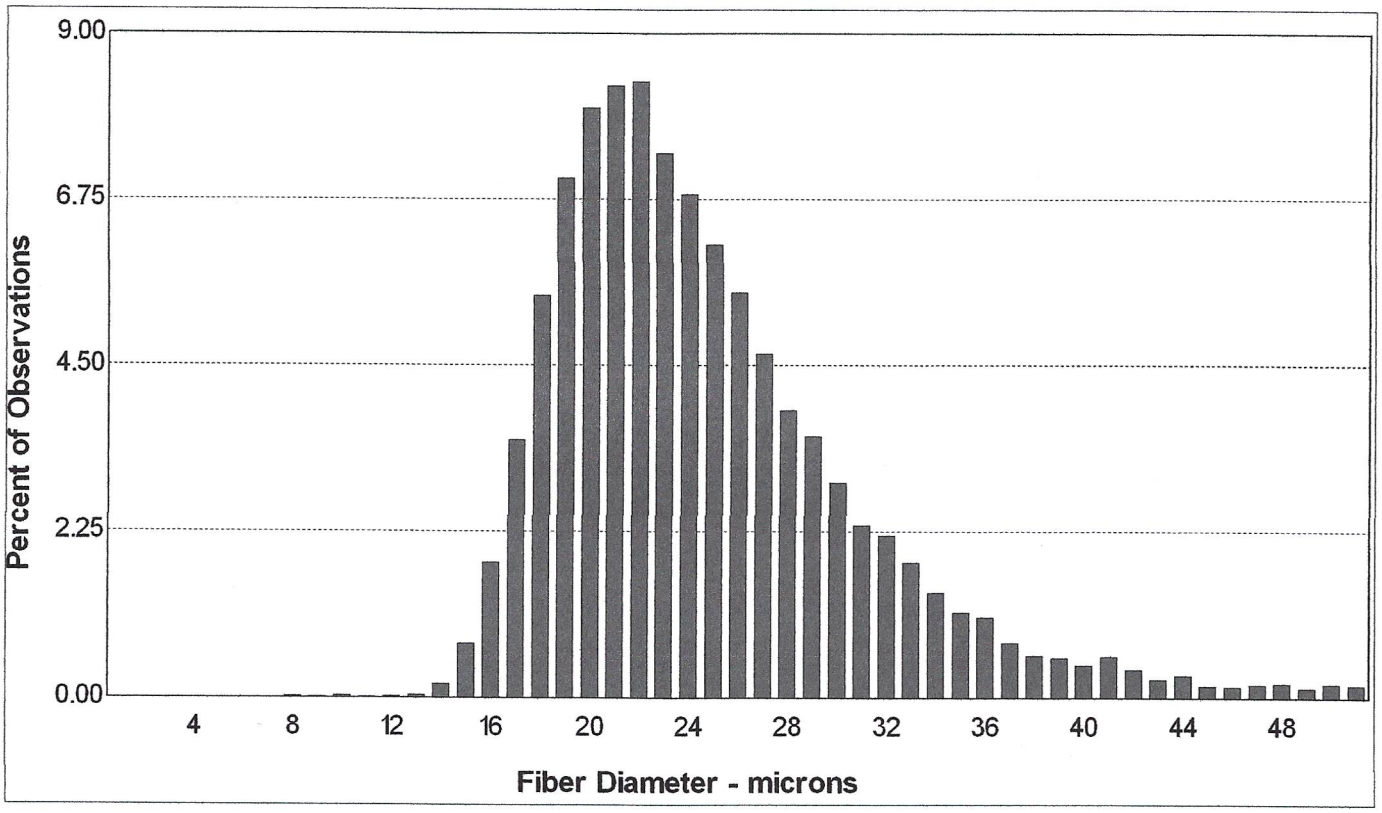

This Test Performed According to I.W.T.O Method 47