Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Willow Wind Farm/Annie Hunt
548 East State Highway 56
Berthoud CO 80513 USA

09/23/17


Test No: 952919

Animal and Sample Description

Animal Name:	Alpacas of NH Ginger Snap	**Animal ID:**	35054108
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Female	**Sample Date:**	05/29/17
Color:	Lt Rose Gray	**Age:**	08/22/15

Laboratory Data

Mean Fiber Diameter:	20.1 microns	**Spin Fineness:**	19.8 microns
Standard Deviation:	4.5 microns	**Mean Curvature (deg/mm):**	48.1
Coefficient of Variation:	22.1 %	**SD Curvature (deg/mm):**	31.9
Fibers Greater Than 30 microns:	2.9 %	**Comfort Factor:**	97.1 %

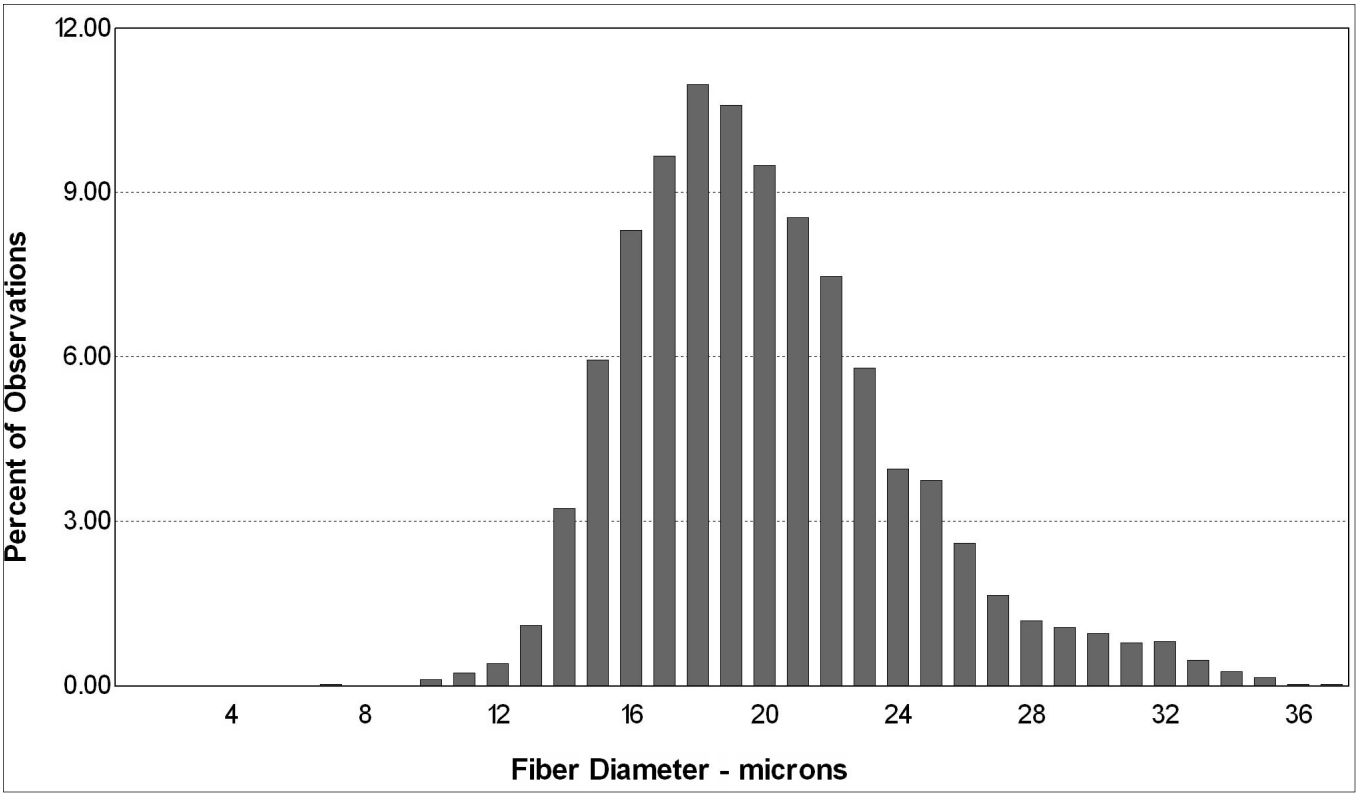

This Test Performed According to I.W.T.O Method 47