



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Heaven's Hill Alpacas/Michael & Alma Gelorme
68 Christy Road
Washington PA 15301 USA

01/16/13

Test No: 449658


Animal and Sample Description

Animal Name: Heaven's Hill Peruvian Callixtus
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Fawn

Animal ID: 31369985
Sample Location: Side
Sample Date: 05/09/12
Age: 09/19/11

Laboratory Data

Mean Fiber Diameter: 17.7 microns
Standard Deviation: 3.3 microns
Coefficient of Variation: 18.7 %
Fibers Greater Than 30 microns: 0.8 %

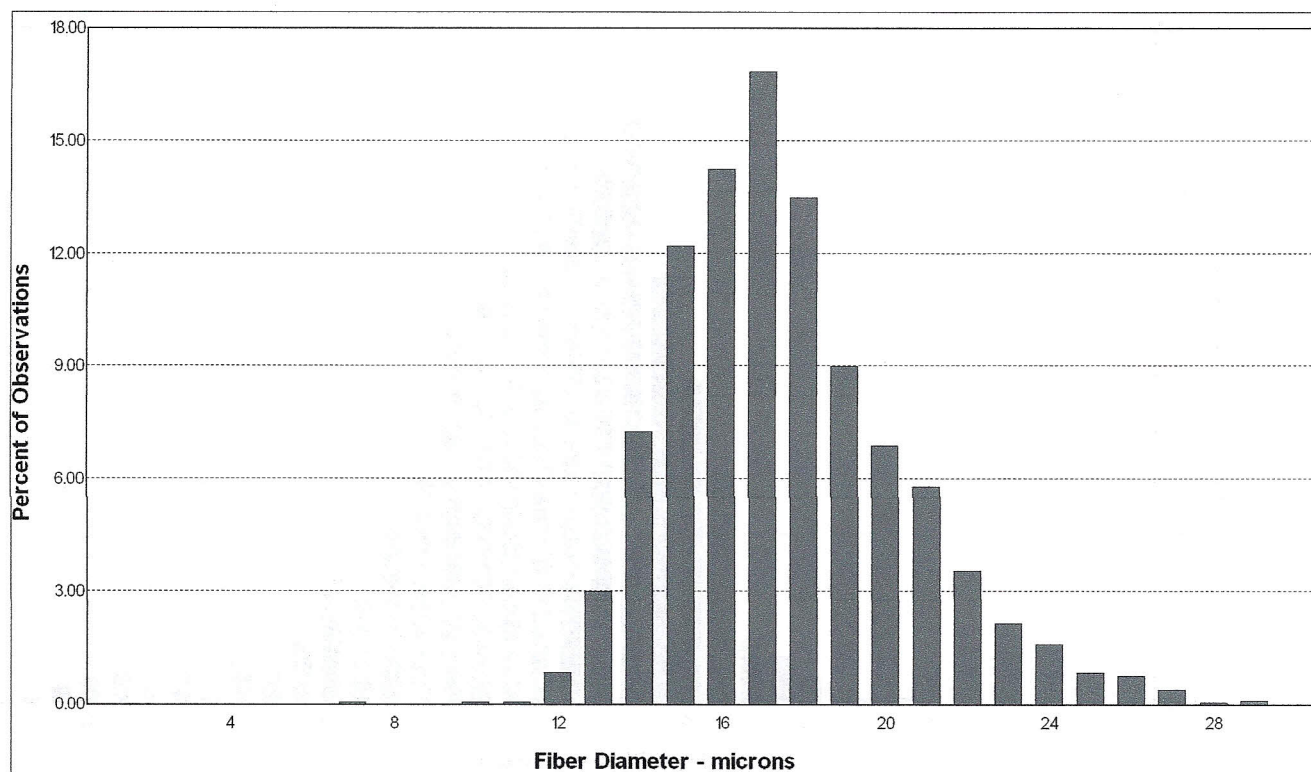

This Test Performed According to I.W.T.O Method 12