Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100)
Micron Test Report

Diversified Alpacas LLC/Jennifer Schalk
1101 West Madison Road
St. Louis MI 48880 USA

Date: 09/28/12


Test No: 446023

Animal and Sample Description

Animal Name:	Mazie	**Animal ID:**	Pending
Breed:	Alpaca(Huacaya)	**Sample Location:**	Side
Sex:	Female	**Sample Date:**	04/22/12
Color:	True Black	**Age:**	06/01/11

Laboratory Data

Mean Fiber Diameter:	20.2 microns	**Fibers Greater Than 30 microns:**	3.4 %
Standard Deviation:	4.7 microns	**Comfort Factor:**	96.6 %
Coefficient of Variation:	23.4 %	**Mean Curvature:**	35.0 deg/mm
Spin Fineness:	20.1 microns	**SD Curvature:**	20.9 deg/mm

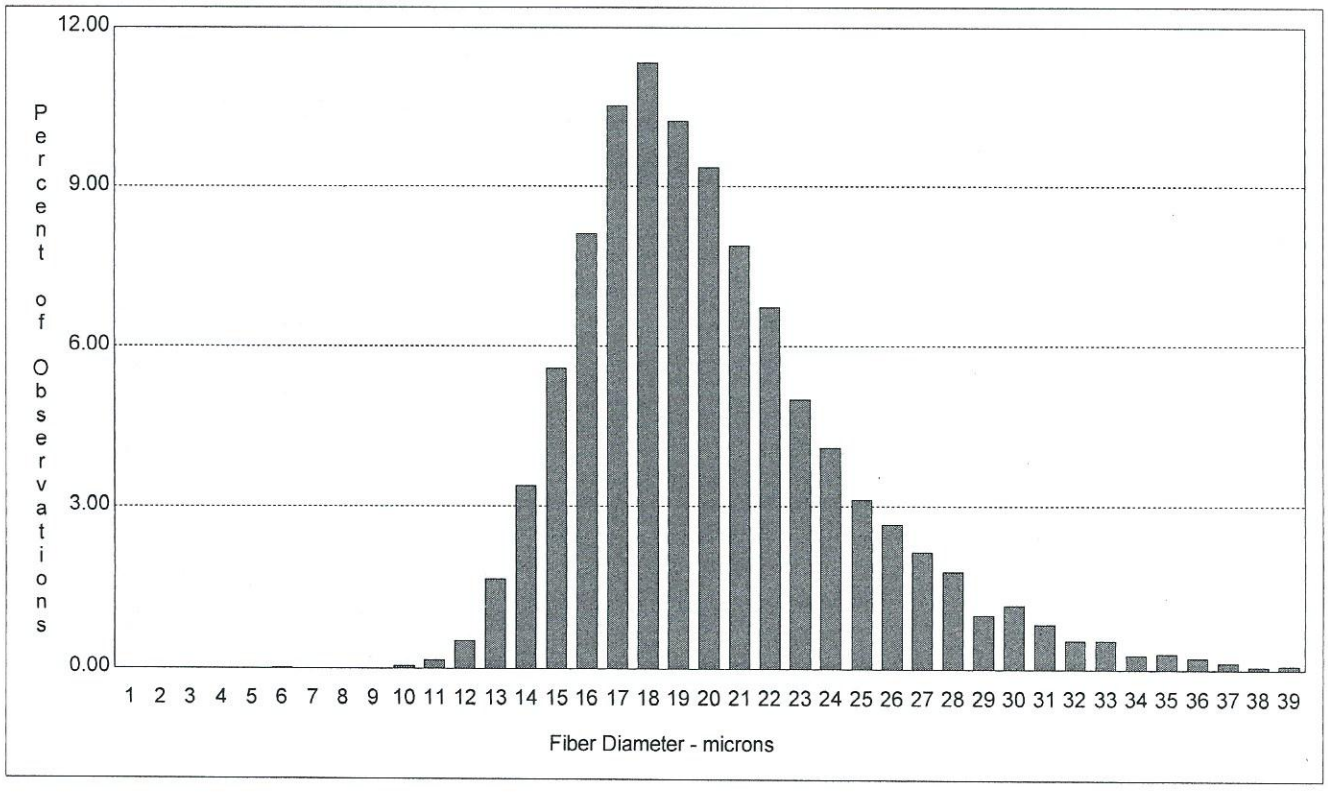

This Test Performed According to I.W.T.O Method 47